

Document No	RP.16.09
Dok. Yayın Tarihi	31.03.2017
Revision No	01
Revision Date	28.06.2022
Page	1 / 1



Background


Male, 37 years old.

Non-smoker.

Non-contributory medical history.

PowerBone Bone Cement LV 20g, Metrosan Dynamic Plate and Titania Hemispherical Polyaxial Screw Hdps 70-40mm products application were performed with the transforminal transdiscal approach to the fracture of the screwed spine of the patient.

Case performed by Prof. Dr. Kemal Yücesoy

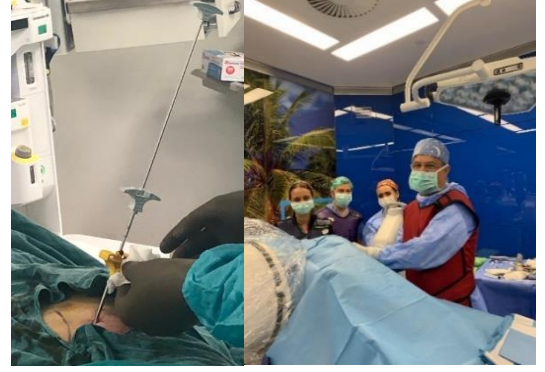

3. Final View.



CASE STUDY

1. Initial radiological view.



2. The Powerbone Bone Cement product is prepared and applied to the area of the spine fracture.



4. You can find more detailed information about the case from the link: <https://pubmed.ncbi.nlm.nih.gov/35817345/>



BONEGRAFT BİYOLOJİK MALZEMELER SAN. VE TİC. A.Ş.
Erzene Mahallesi Ankara Cad. No:172/67
Ege Üniversitesi Sit İdege Teknoloji Geliştirme
Bölgesi BORNOVA / İZMİR / TÜRKİYE
www.bonegraft.com.tr/
info@bonegraft.com.tr