

Document No	RP.16.09
Dok. Yayın Tarihi	31.03.2017
Revision No	01
Revision Date	28.06.2022
Page	1 / 2



Background

Female, 16 years old.

Metrosan-Ligamed Posterior Polyaxial Spine Stabilization Screw 5,5x35/ 5,5x40/ 5,5x45


-Metrosan-Ligamed Polyaxial reduction screw 5,5x35/ 5,5x40/ 4,5x30/ 4,5x25

-Metrosan-Ligamed Titanium Rod 55x450mm

-Powerbone Flexible Graft were used for the patient with scoliosis due to cerebral palsy disease.


Case performed by Doç. Dr. Mehmet ÇETİNKAYA- Orthopedic Spine Surgeon

2. Metrosan-Ligamed Posterior Polyaxial Spine Stabilization Screws, Titania Polyaxial Reduction Screw, Titanium Rod and Powerbone Flexible Graft products were used with surgical intervention to treat scoliosis.

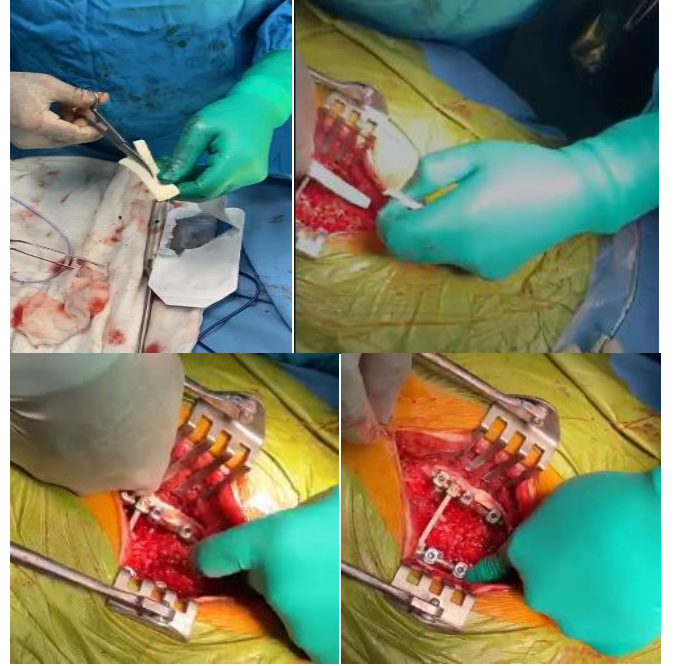


CASE STUDY

1. Initial radiological view.

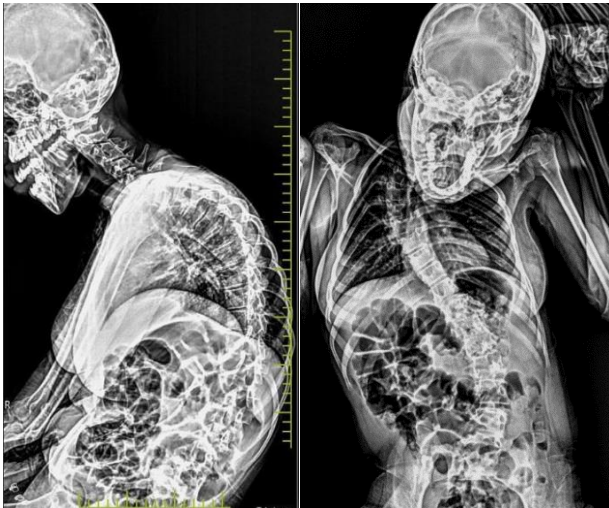


Document No	RP.16.09
Dok. Yayın Tarihi	31.03.2017
Revision No	01
Revision Date	28.06.2022
Page	2 / 2

3. Post-operation radiological view.

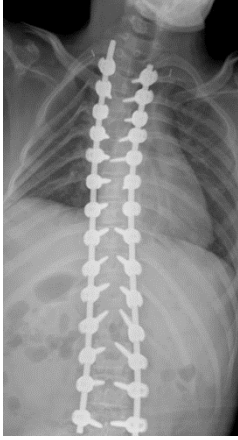

4. Before and after radiological view.

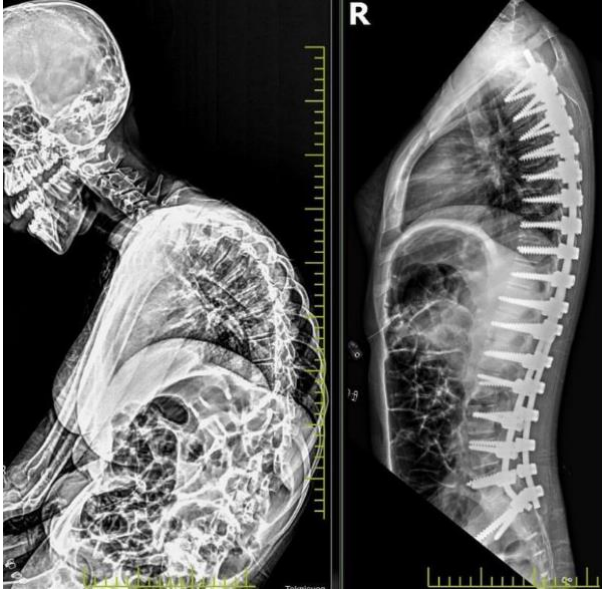

**BONEGRAFT BİYOLOJİK MALZEMELER SAN. VE
TİC. A.Ş.**

Erzene Mahallesi Ankara Cad. No:172/67
Ege Üniversitesi Sit İdege Teknoloji
Geliştirme Bölgesi BORNOVA / İZMİR /
TÜRKİYE

www.bonegraft.com.tr/ •
info@bonegraft.com.tr